

CERTIFICAT D'ETALONNAGE No 15M-007548

KALIBRIERSCHEIN

CALIBRATION CERTIFICATE

Messuhr Comparateur Dial Indicator

No de série  
Seriennummer  
Serial Number

12399046

Course de mesure  
Meßspanne  
Measuring Range

100 mm

Résolution  
Auflösung  
Resolution

0.001 mm

Force de mesure  
Messkraft  
Measuring Force

1.60 - 3.50 N

Précourse  
Anhub  
Pretravel

0.200 mm


Etalonné avec  
Kalibriert  
Calibrated with

Laser 1943 / METAS Nr 111-05732

Nous certifions que cet instrument a été fabriqué et contrôlé selon ses normes internes de Qualité.  
Les étalons utilisés ont une traçabilité reconnue par METAS (Office Fédéral de METrologie et Accréditation Suisse).

Wir bestätigen, dass dieses Instrument gemäss seinen internen Qualitätsnormen hergestellt und geprüft wurde.  
Die verwendeten Referenzmasse verfügen über eine anerkannte Rückverfolgbarkeit durch METAS (Eidgenössische Amt METrologie und Akkreditierung Schweiz).

We certify that this instrument has been manufactured according to our Standard of Quality and tested in reference with master of certified traceability by METAS (federal office of METrology and Accreditation Switzerland).

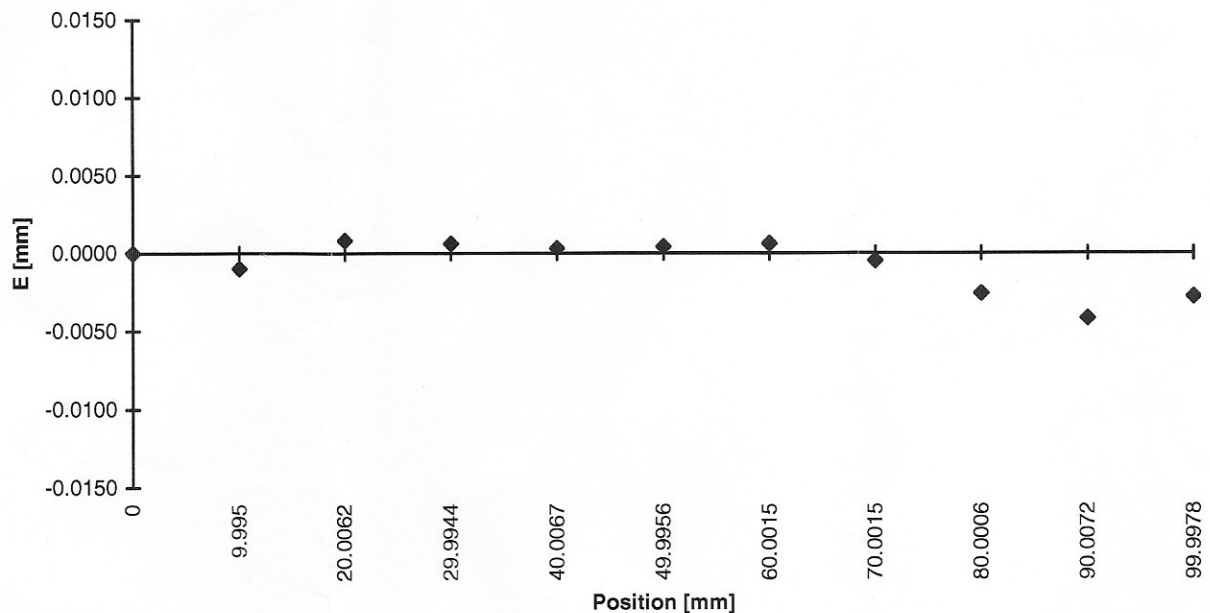

Erreur Maximum  
Maximale Abweichung  
Maximum Error

5  $\mu$ m

Incertitude de mesure (U95%)  
Uncertainty of measurement (U95%)  
Messunsicherheit (U95%)

0.95  $\mu$ m

Contrôleur / Prüfer / Inspector

.....*J. Silva*.....

26.09.2012